Quick Reference Guide

DART™ Drug Atomizing Recovery Tool

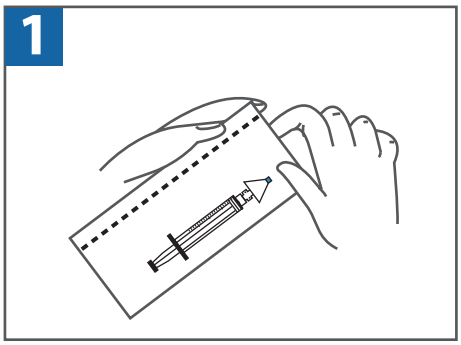

Remove the DART from the packaging.

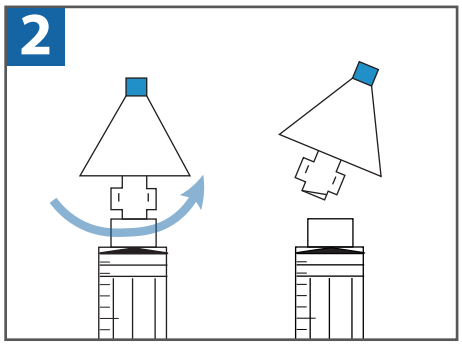

Remove the Nasal atomizer by twisting it counter clockwise.

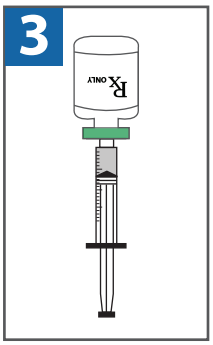

Add the desired medication to the syringe.

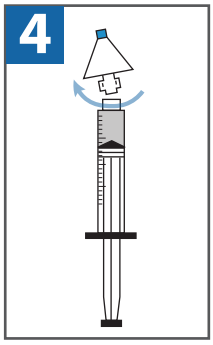

Reattach the Nasal device to the syringe (turn clockwise.)

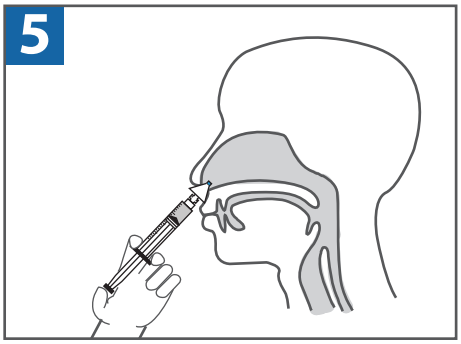

Place the tip of the device into the patients nostril. The device should be pointing slightly up and laterally (towards the tip of the patients ear on the same side of the head).

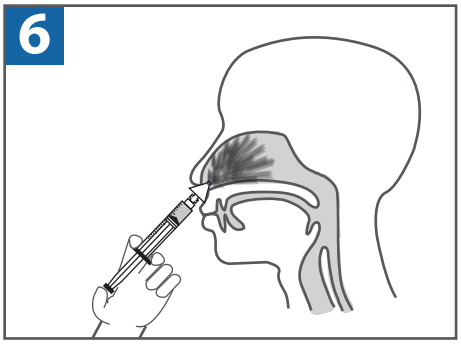

Compress the syringe plunger briskly until half the dose enters one nostril, repeat on the opposite side to administer the remaining medication.

7. Titrate to clinical effect in 5-15 minutes with another appropriate dose of medication if indicated.

DART100 - DART Nasal Device with 3mL Syringe

DART300 - DART Nasal Device without Syringe

Additional Tips:

- Compress the Syringe with a brisk pressure to maximize the atomization.
- Utilize both nostrils to increase the treated surface area.

Contraindications:

- Mucous, blood, and vascoconstrictors reduce absorption of medication.

Pulmodyne®

For additional information regarding the DART
Visit our website at **www.pulmodyne.com** or call **317.900.4093**